


FIG. 1A

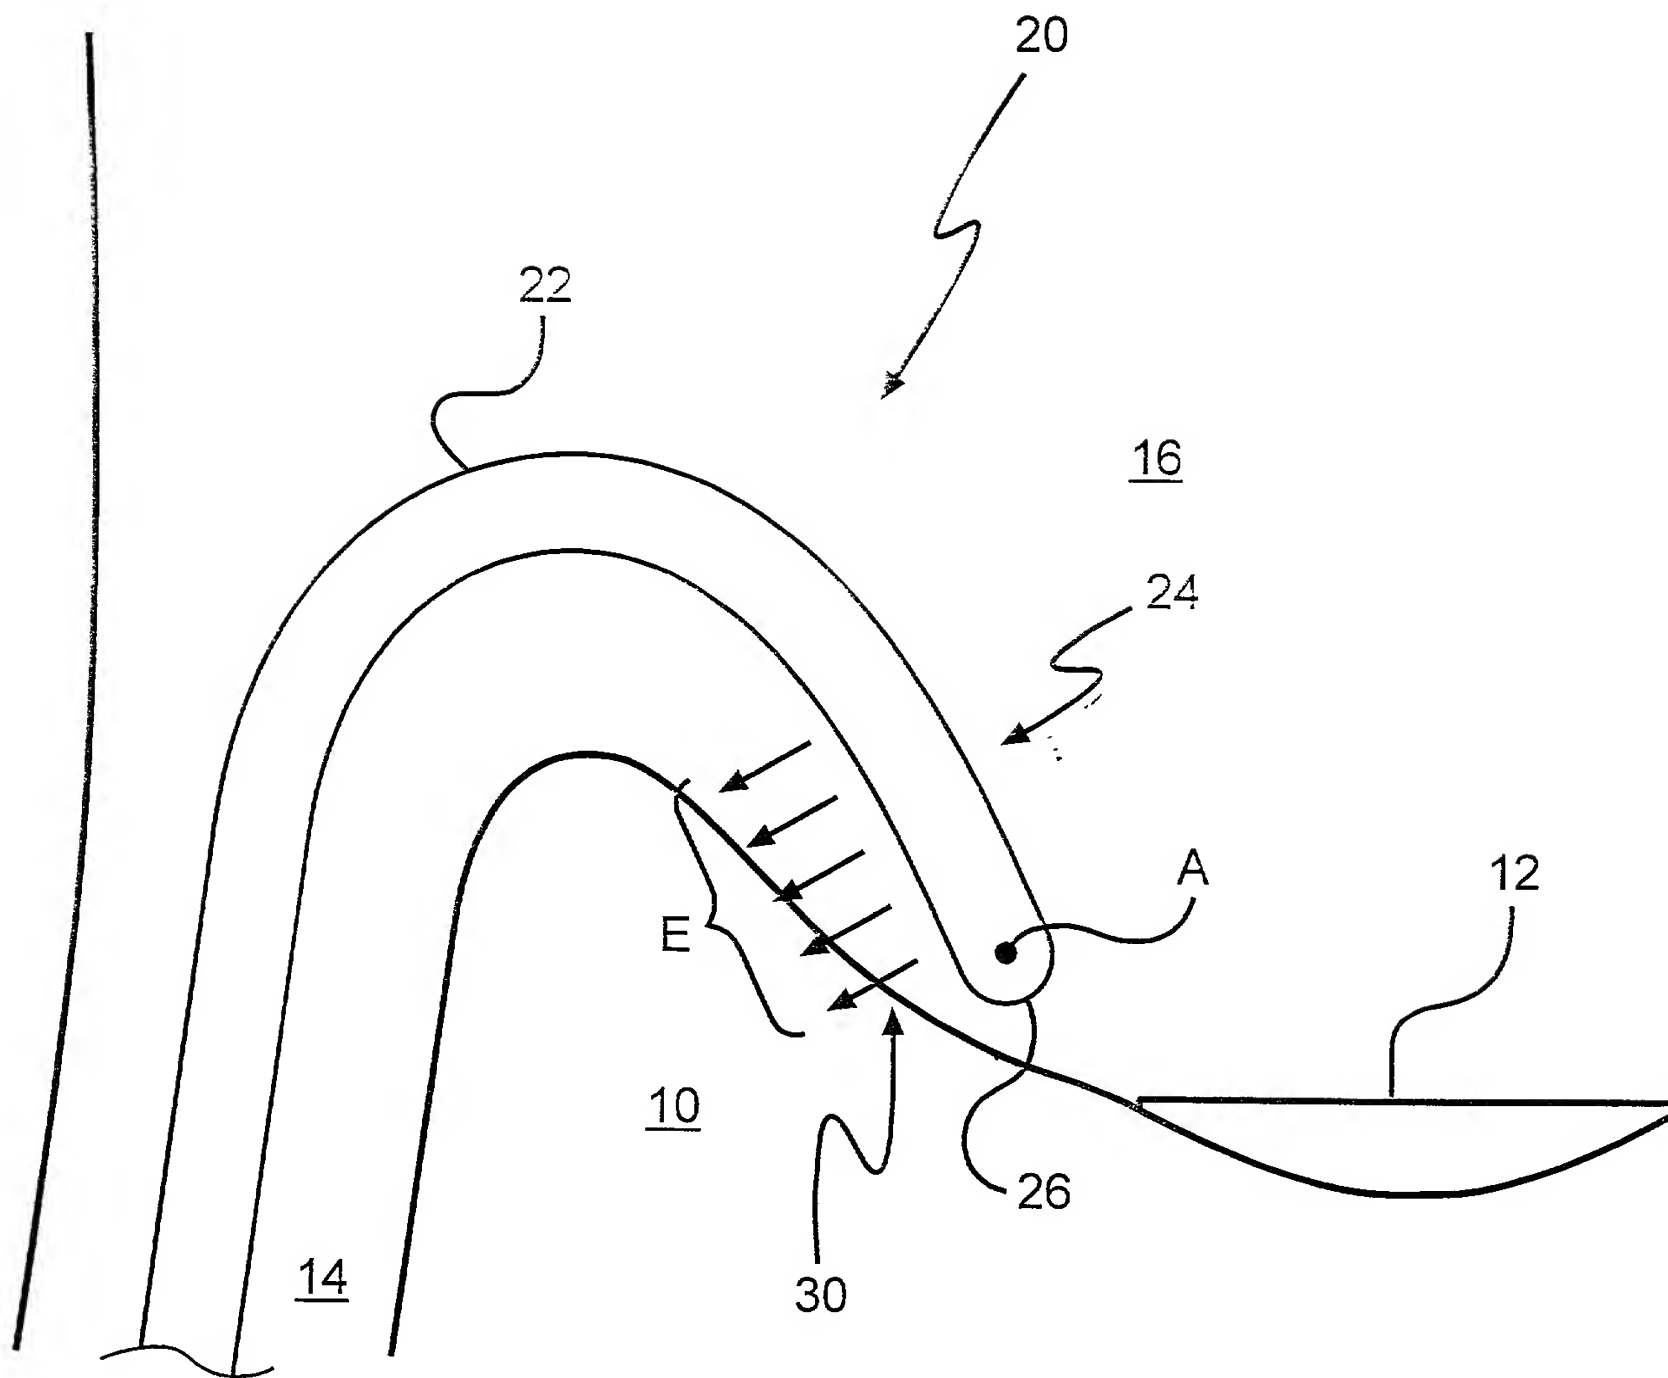

**FIG. 1A**

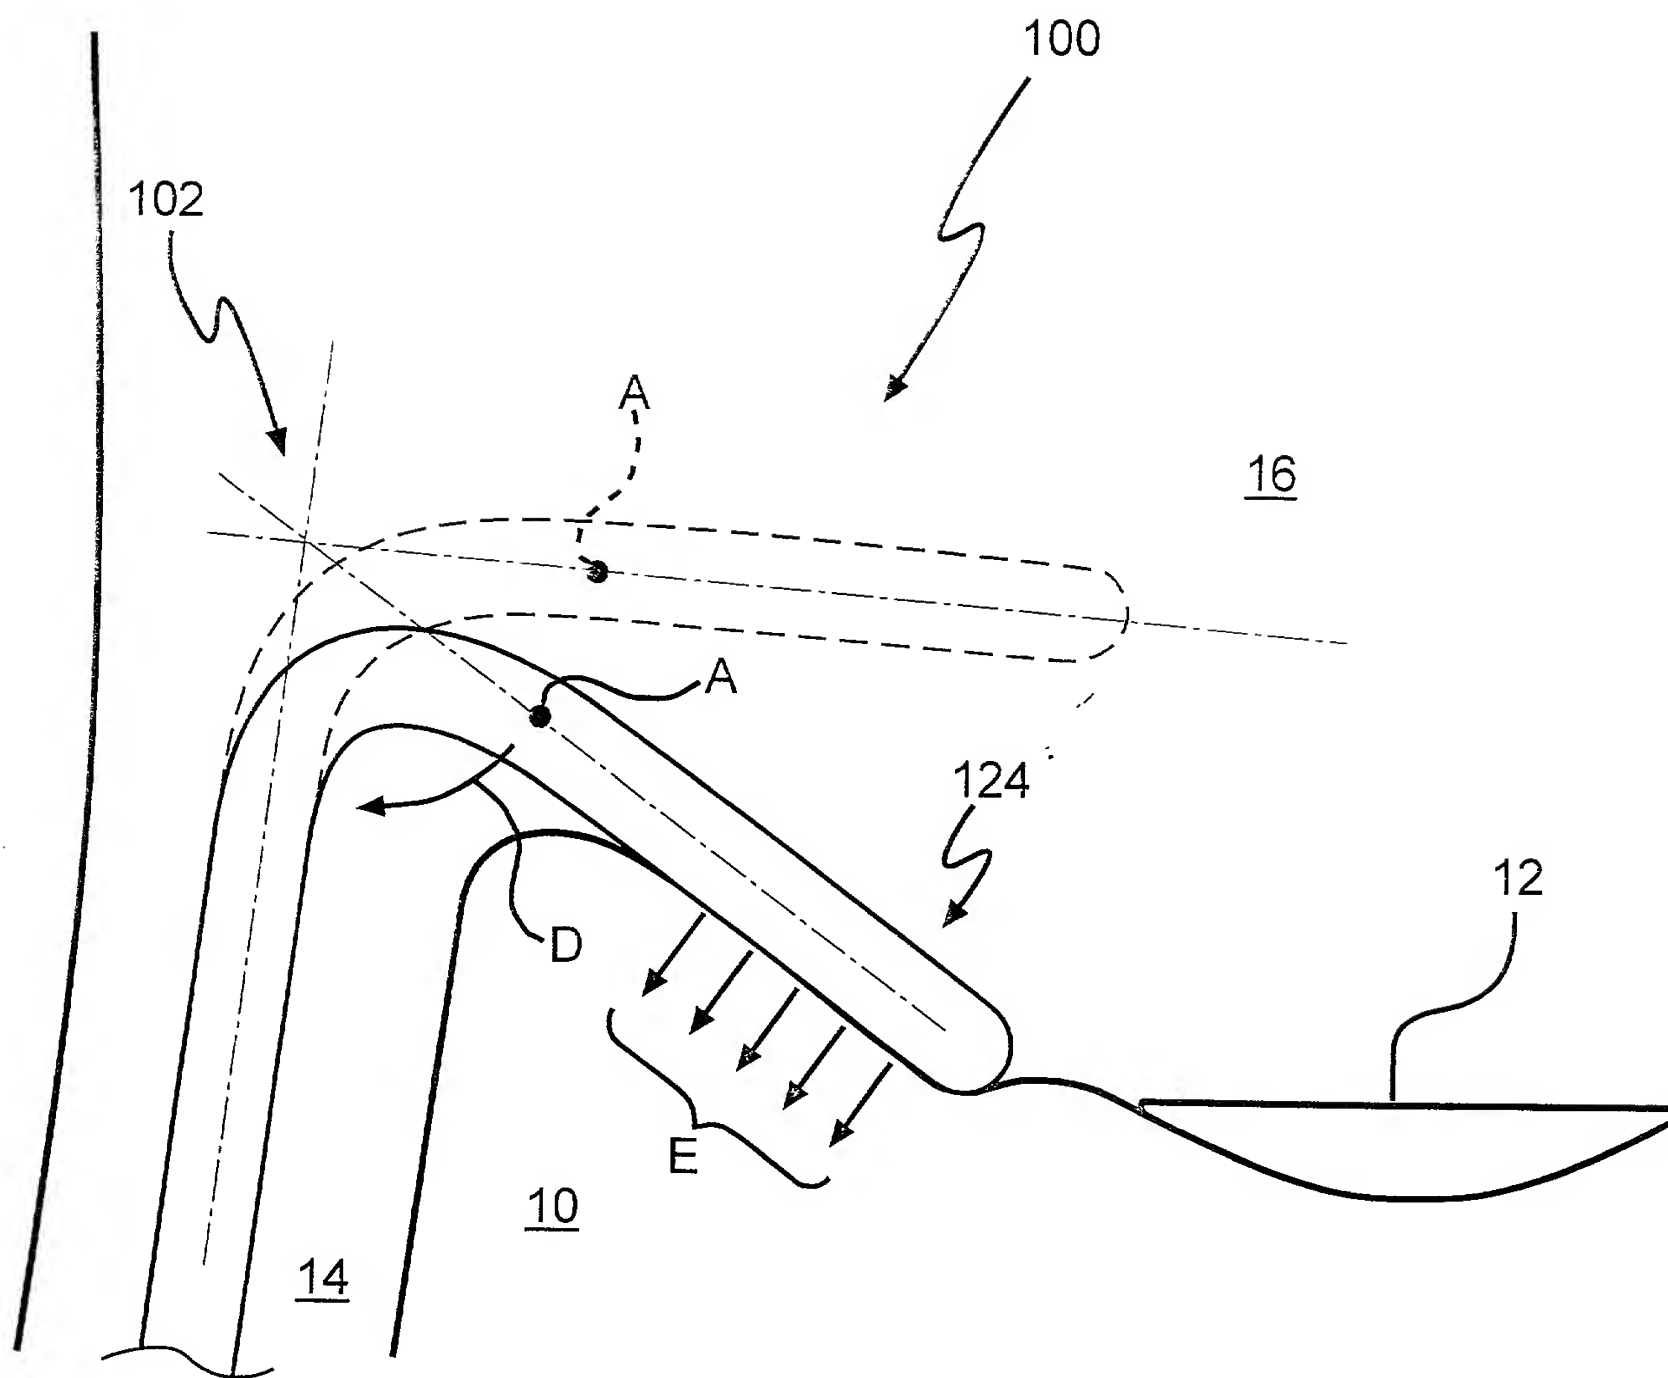


FIG. 1B

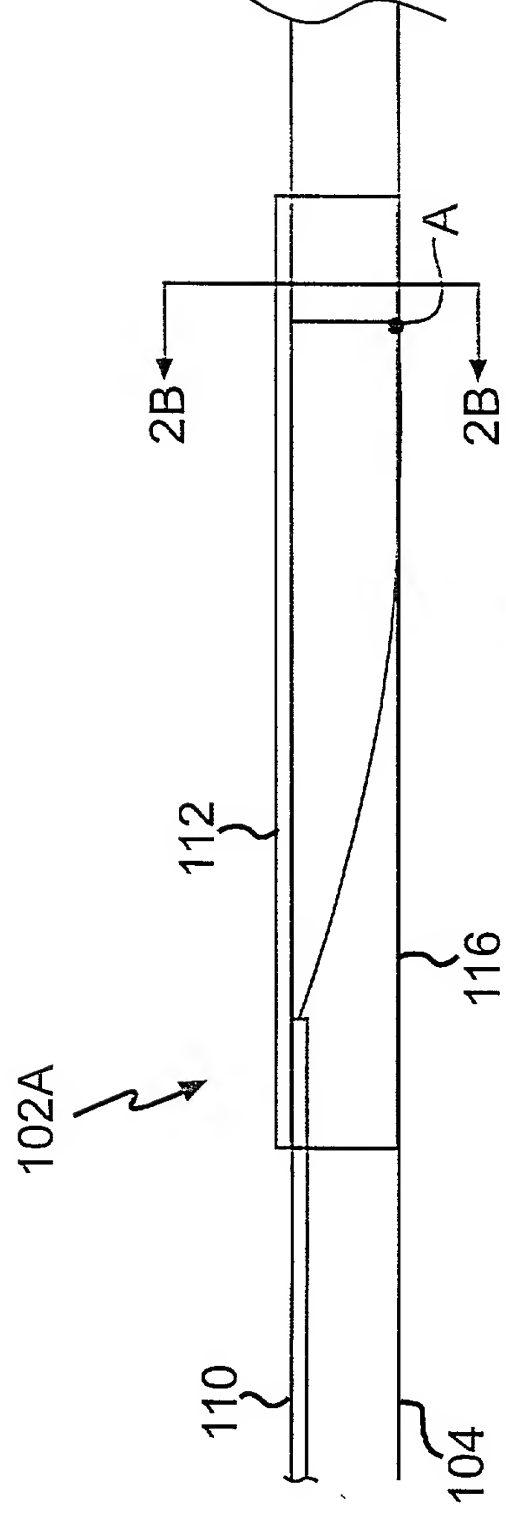


FIG. 2A



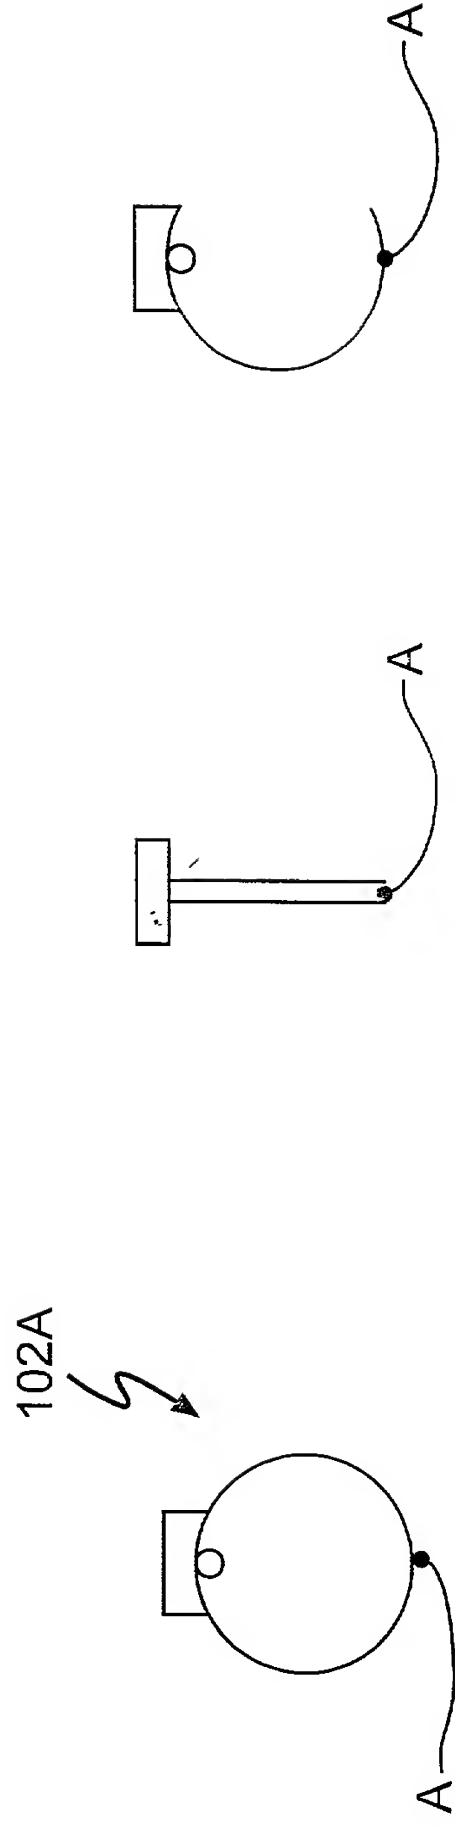


FIG. 2B

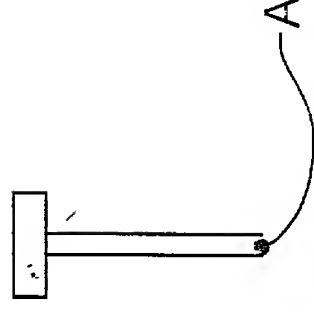

**FIG. 2**

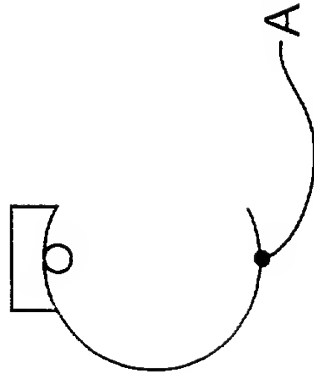

**FIG. 2D**

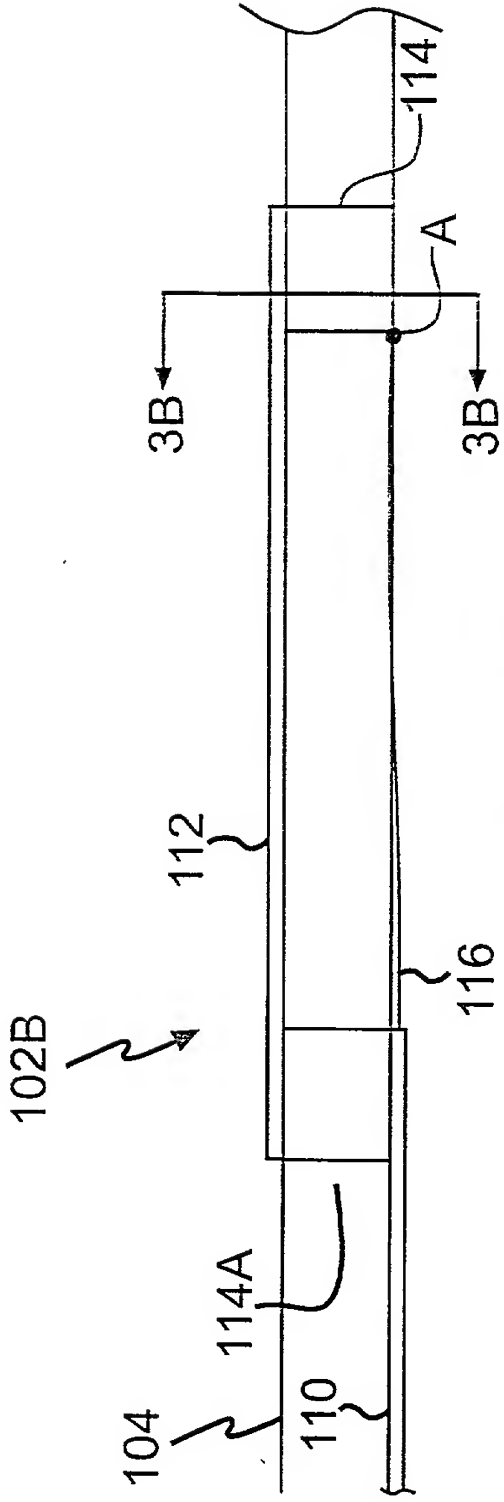


FIG. 3A


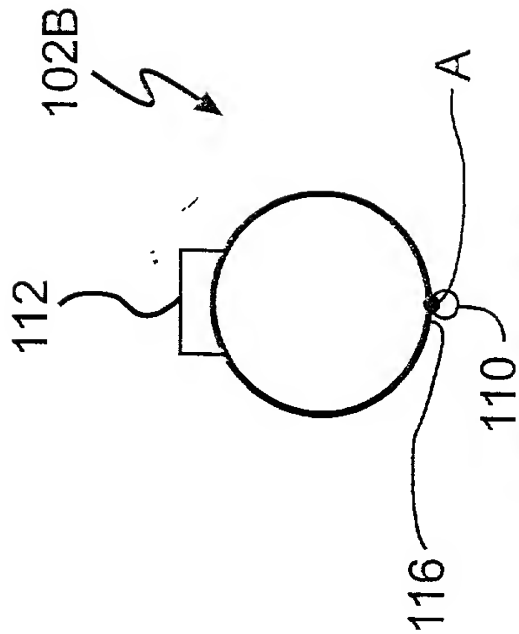


FIG. 3B

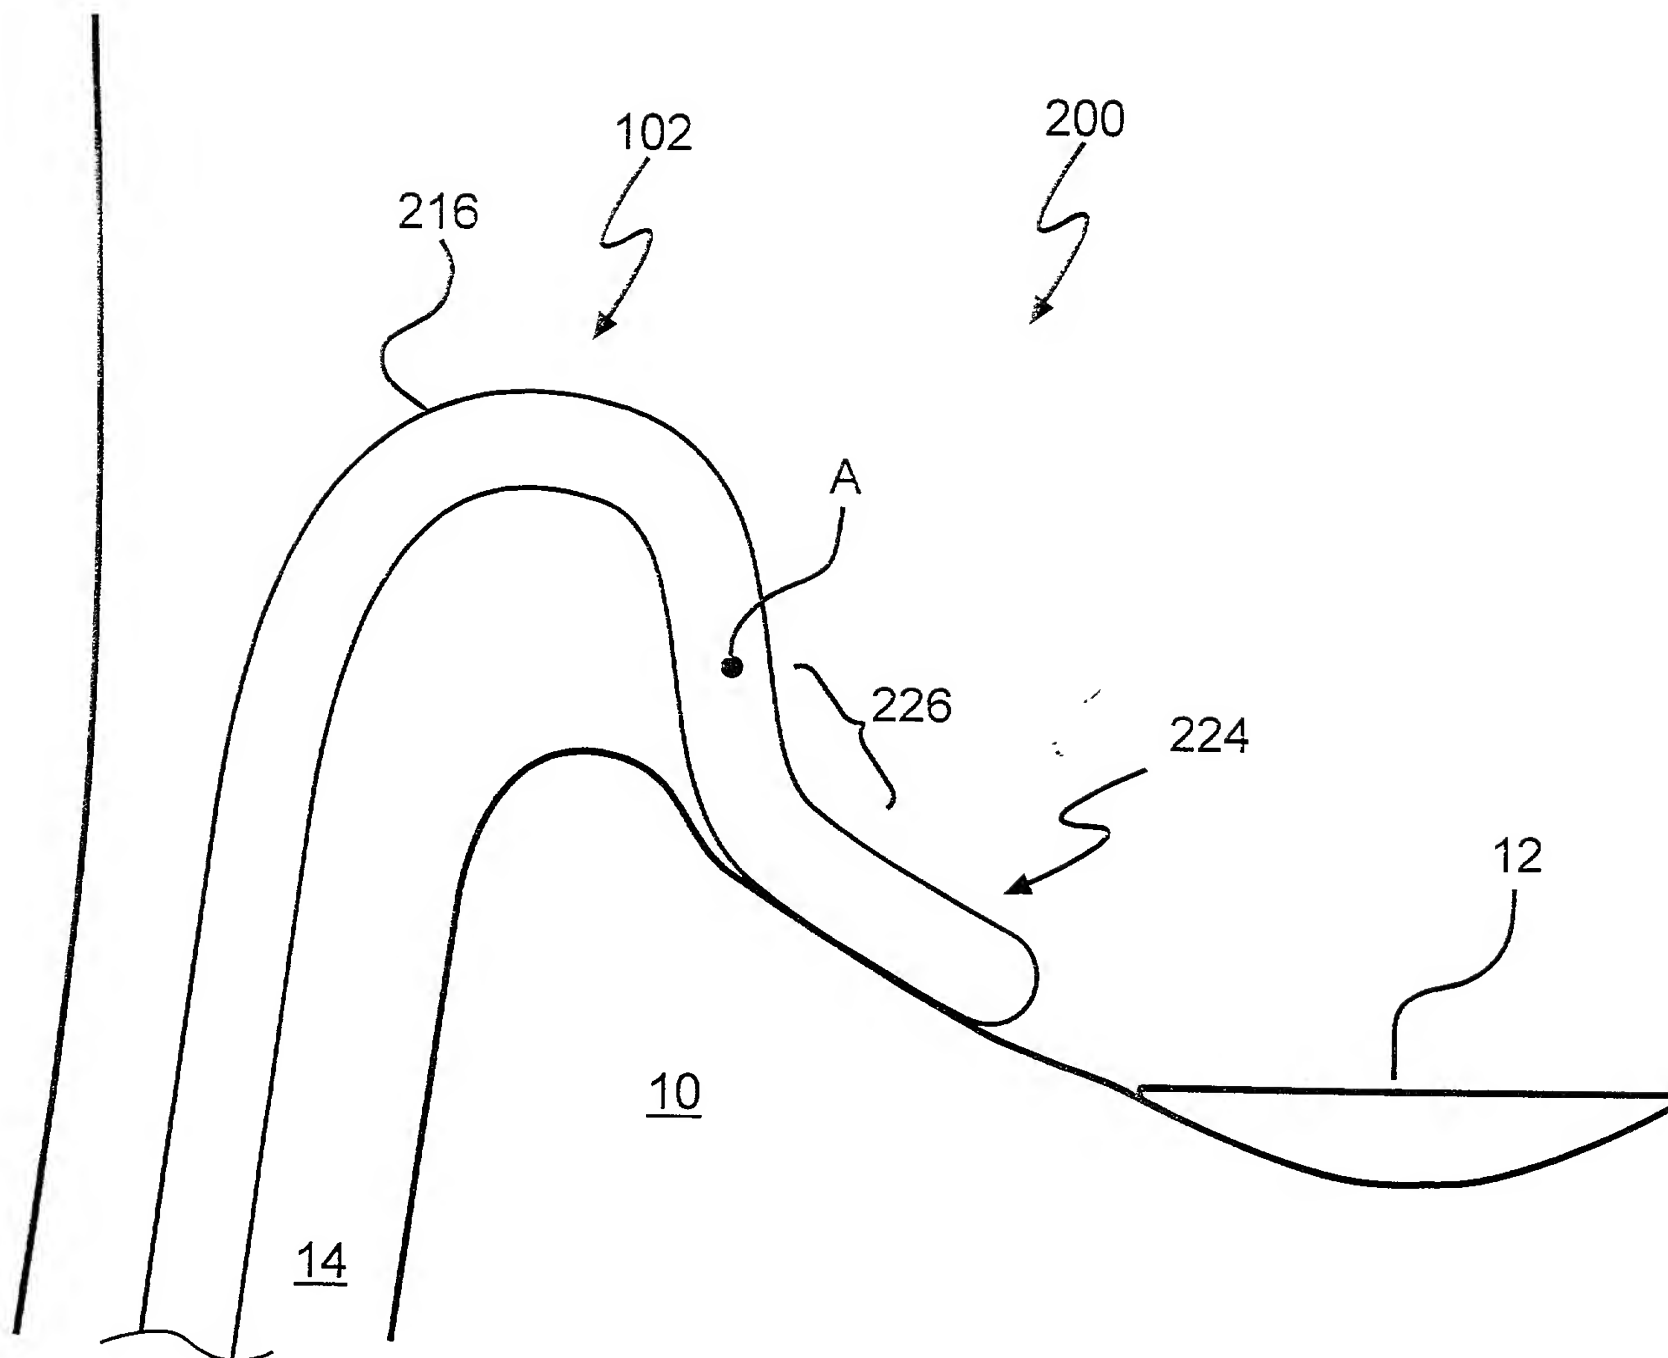

**FIG. 4**

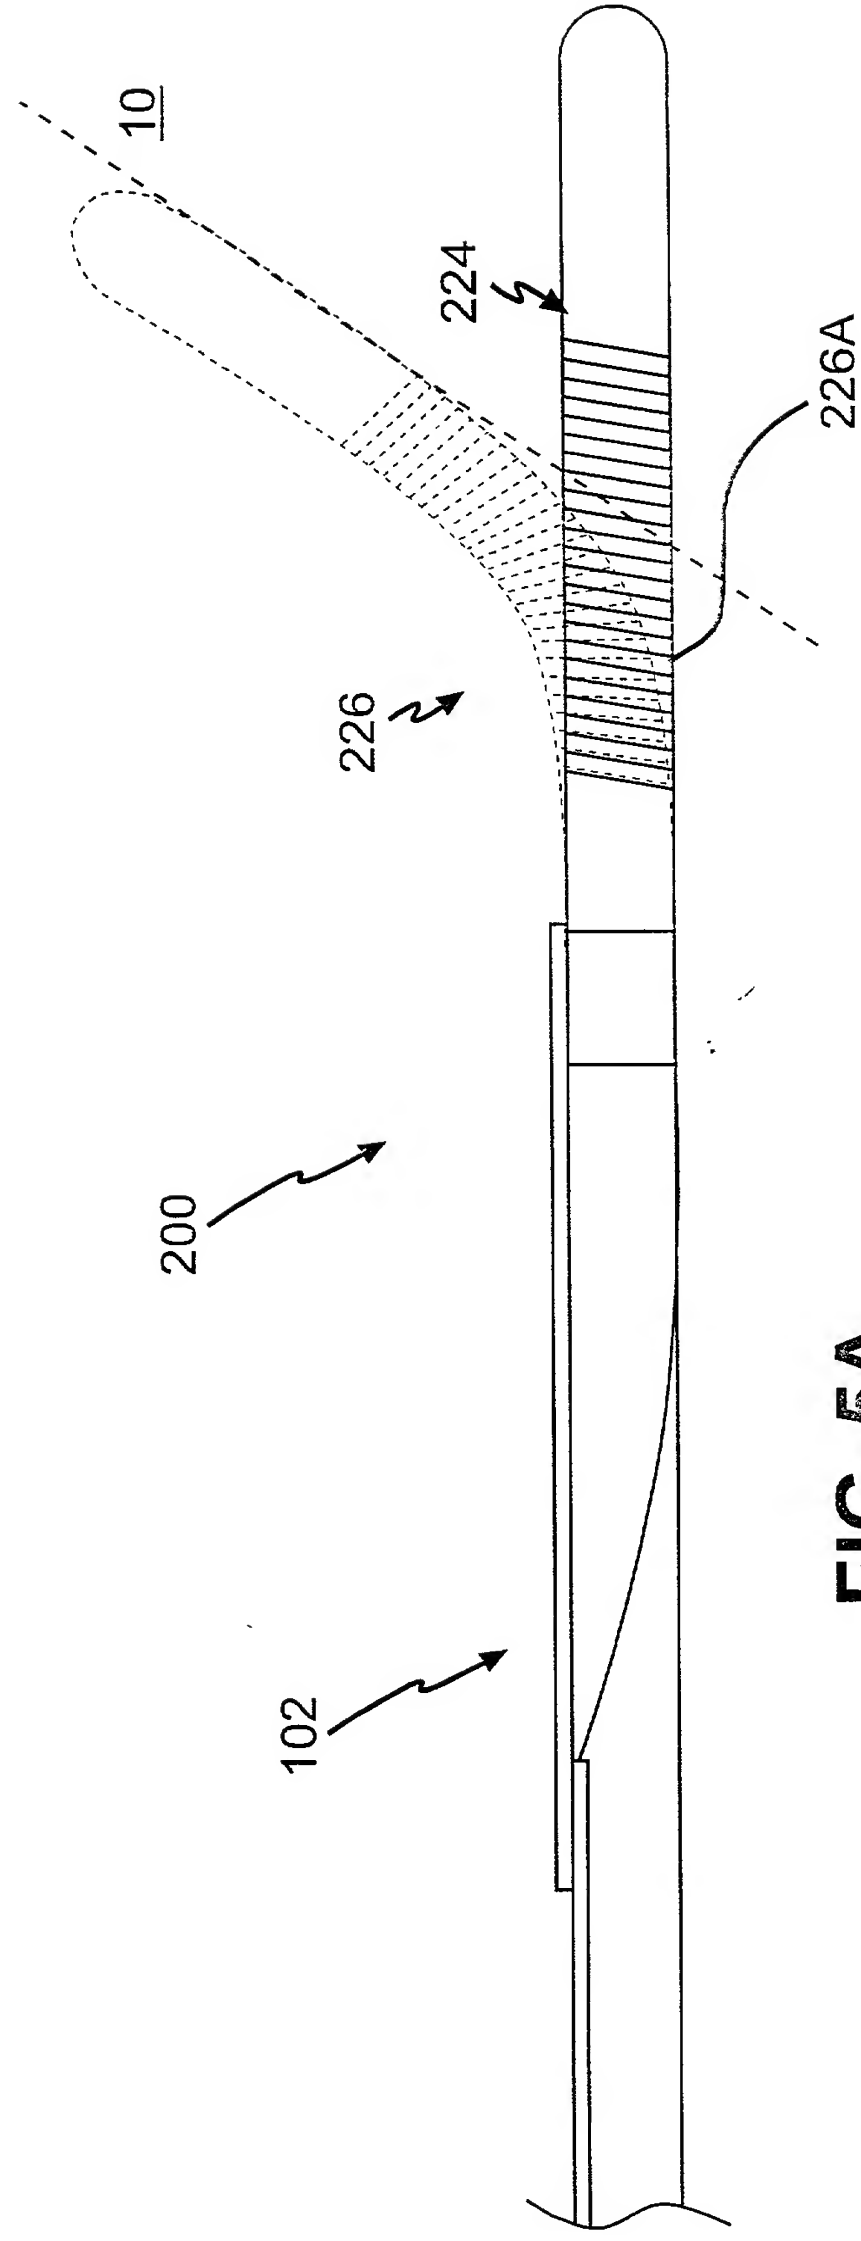


FIG. 5A

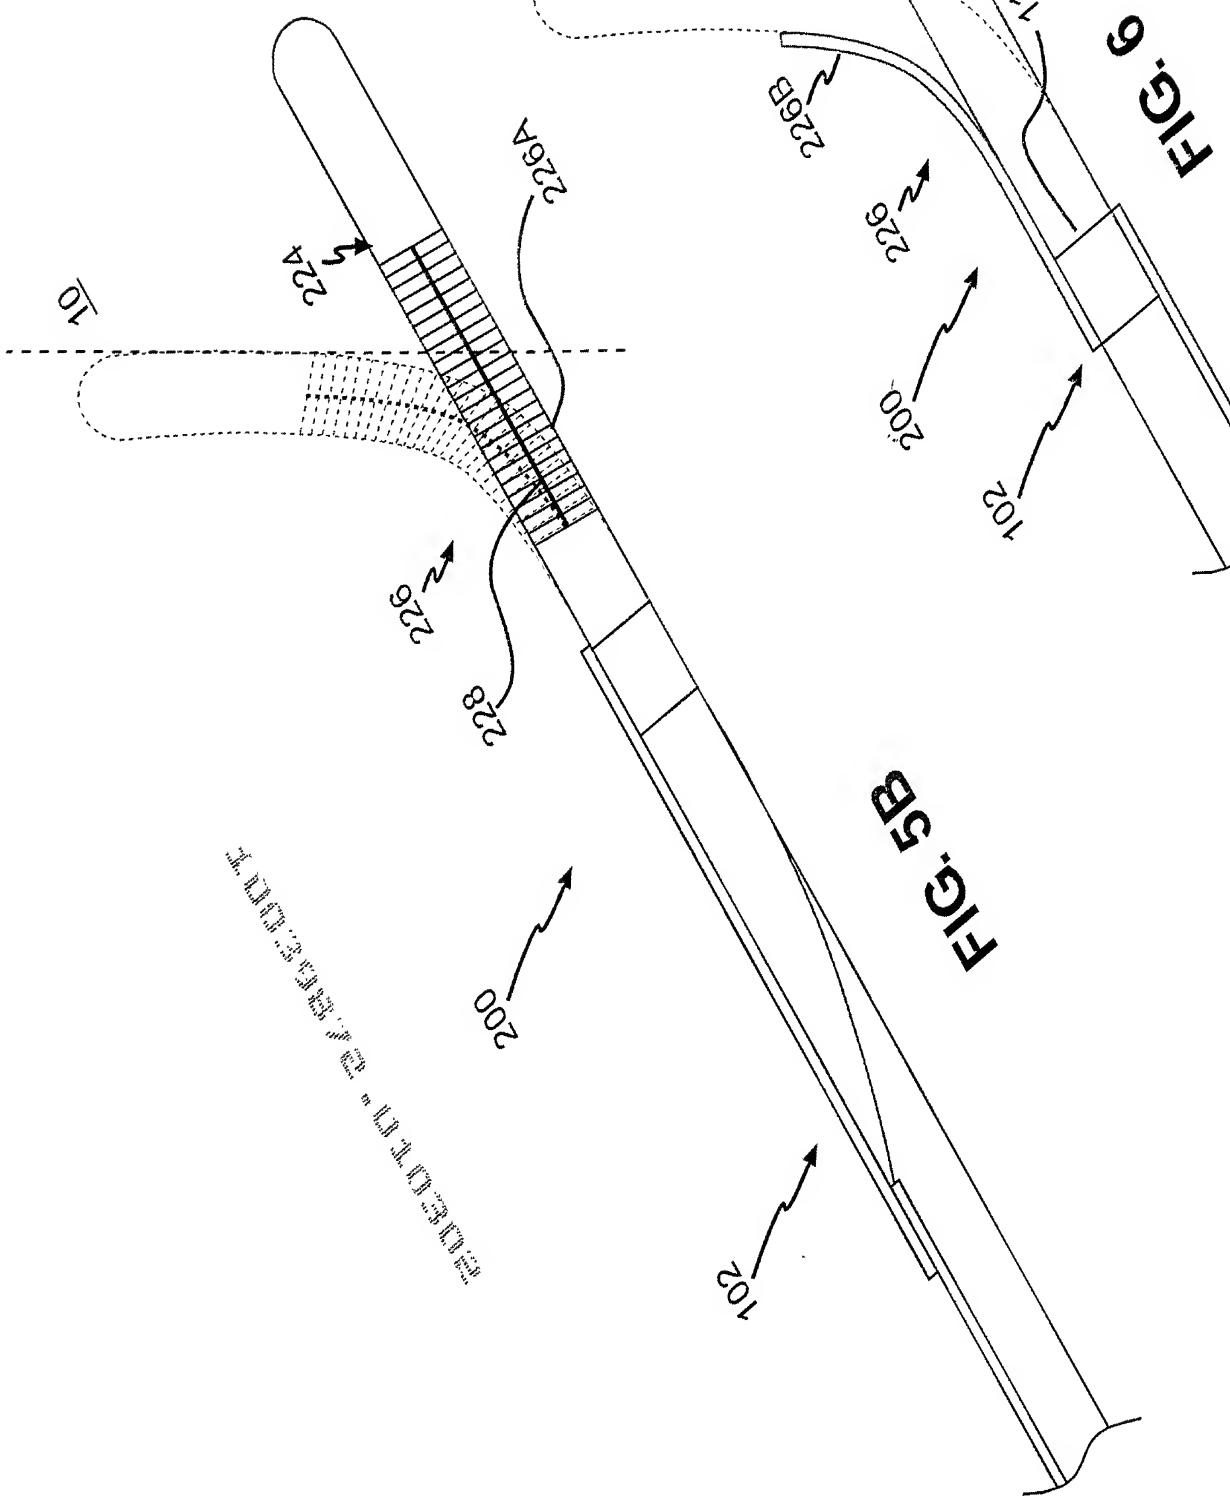
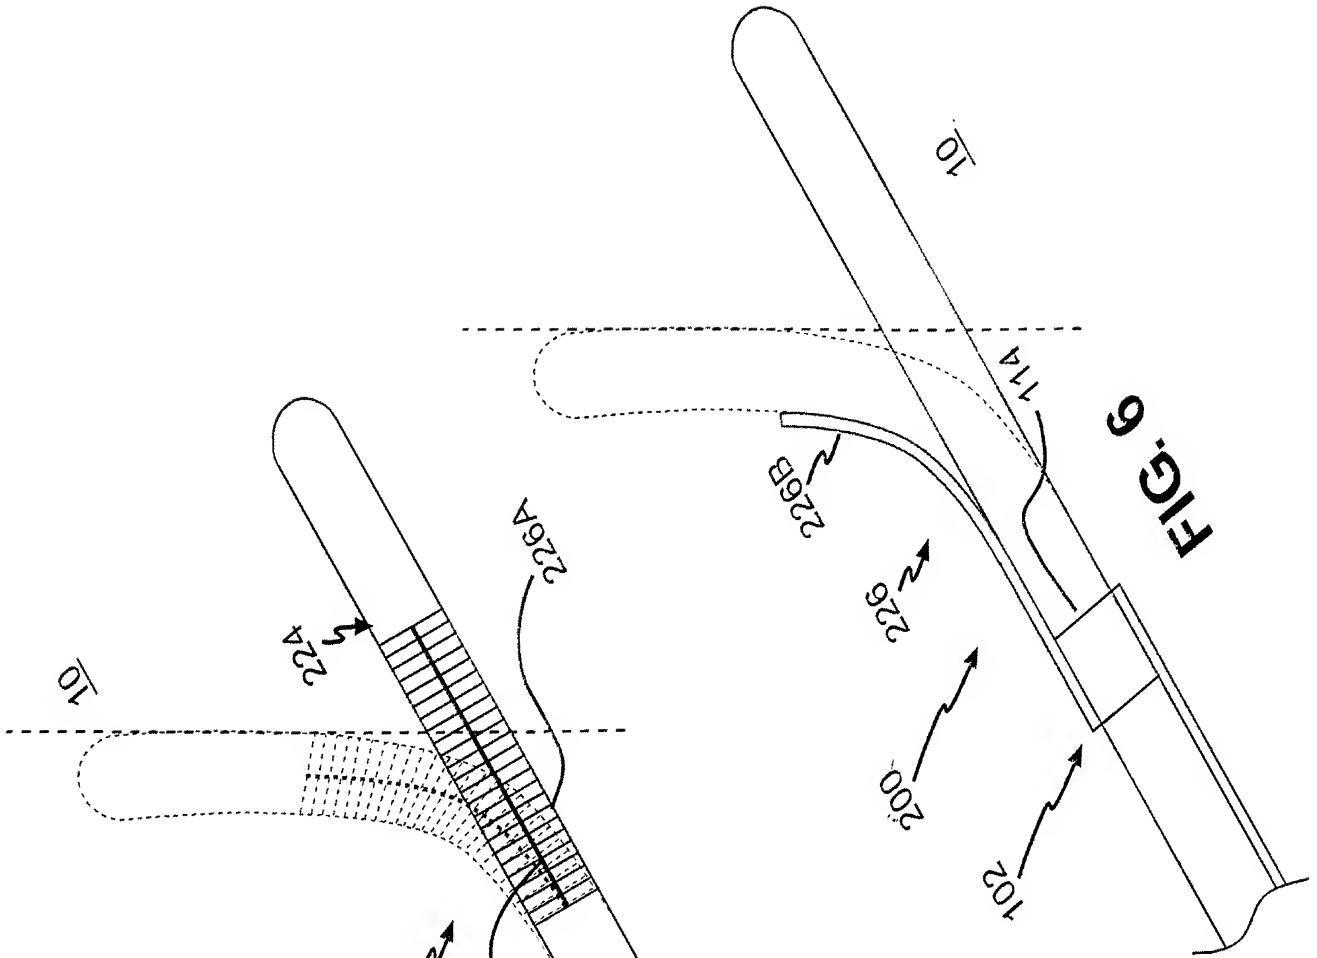


FIG. 5B is a perspective view of the device 10 in a second configuration, showing the curved member 200 in a different position relative to the handle 102 and the distal tip 114. The dashed line A-A indicates a cross-section through the device.

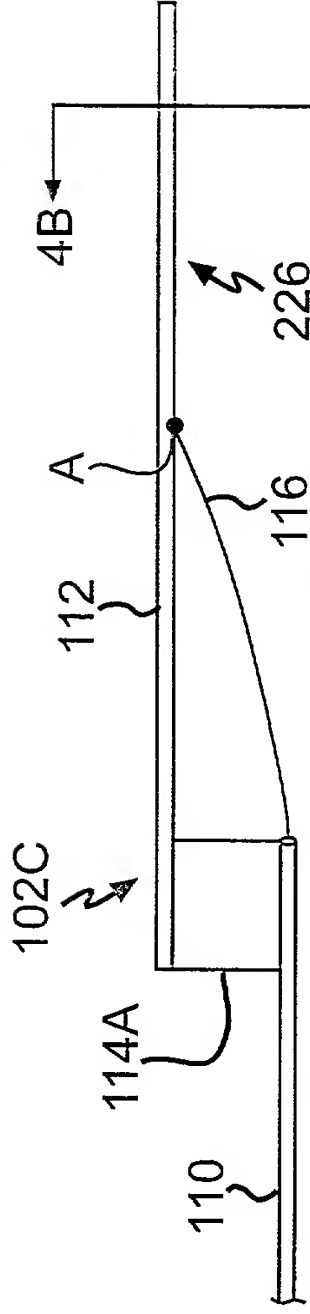


FIG. 7A




FIG. 7B

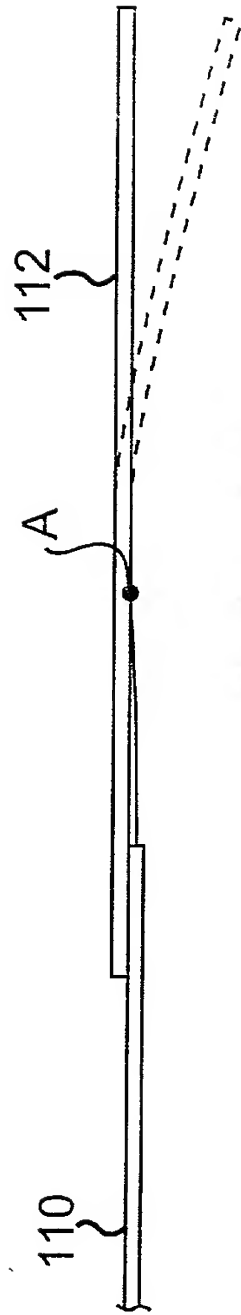


FIG. 8A






FIG. 8B

FIG. 9A

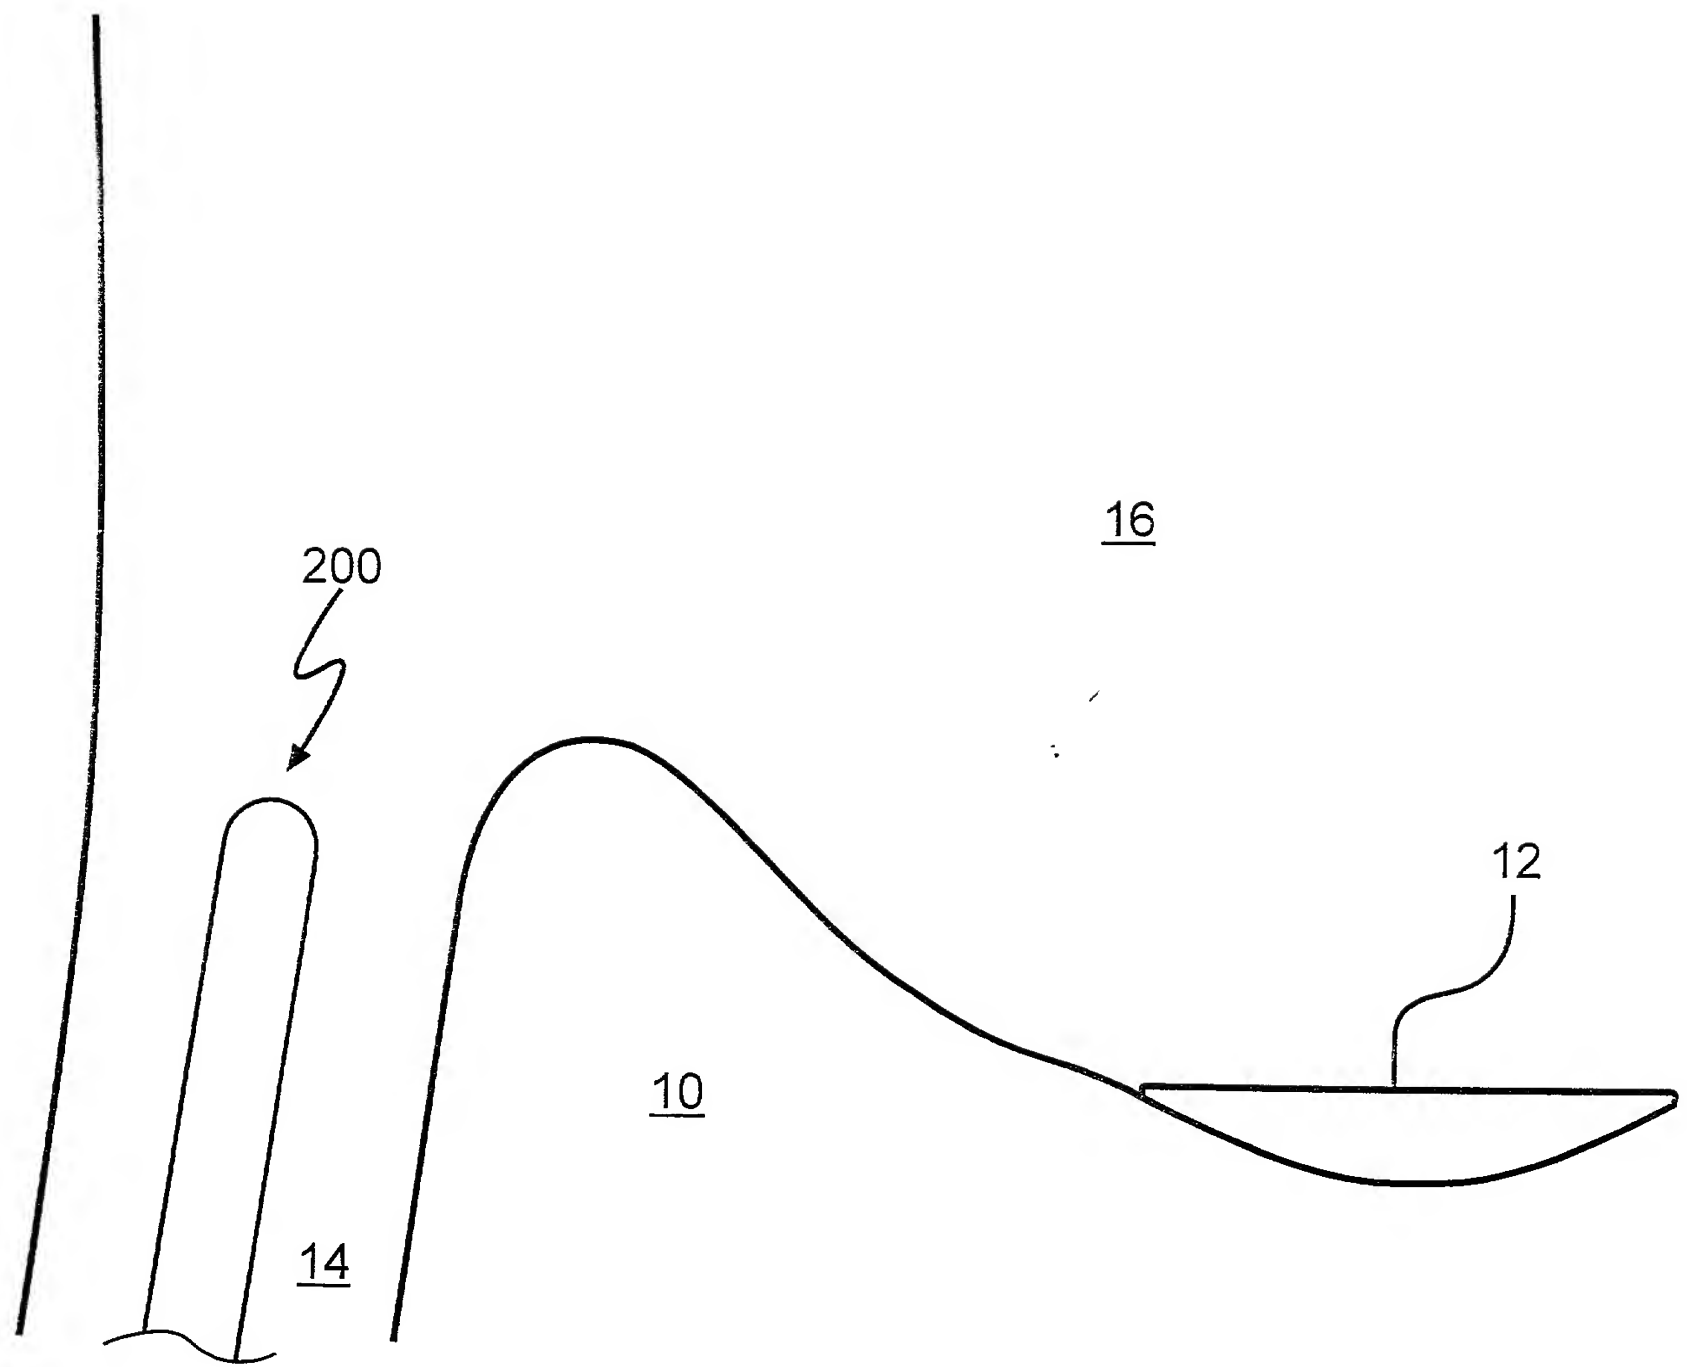


**FIG. 9A**

FIG. 9B

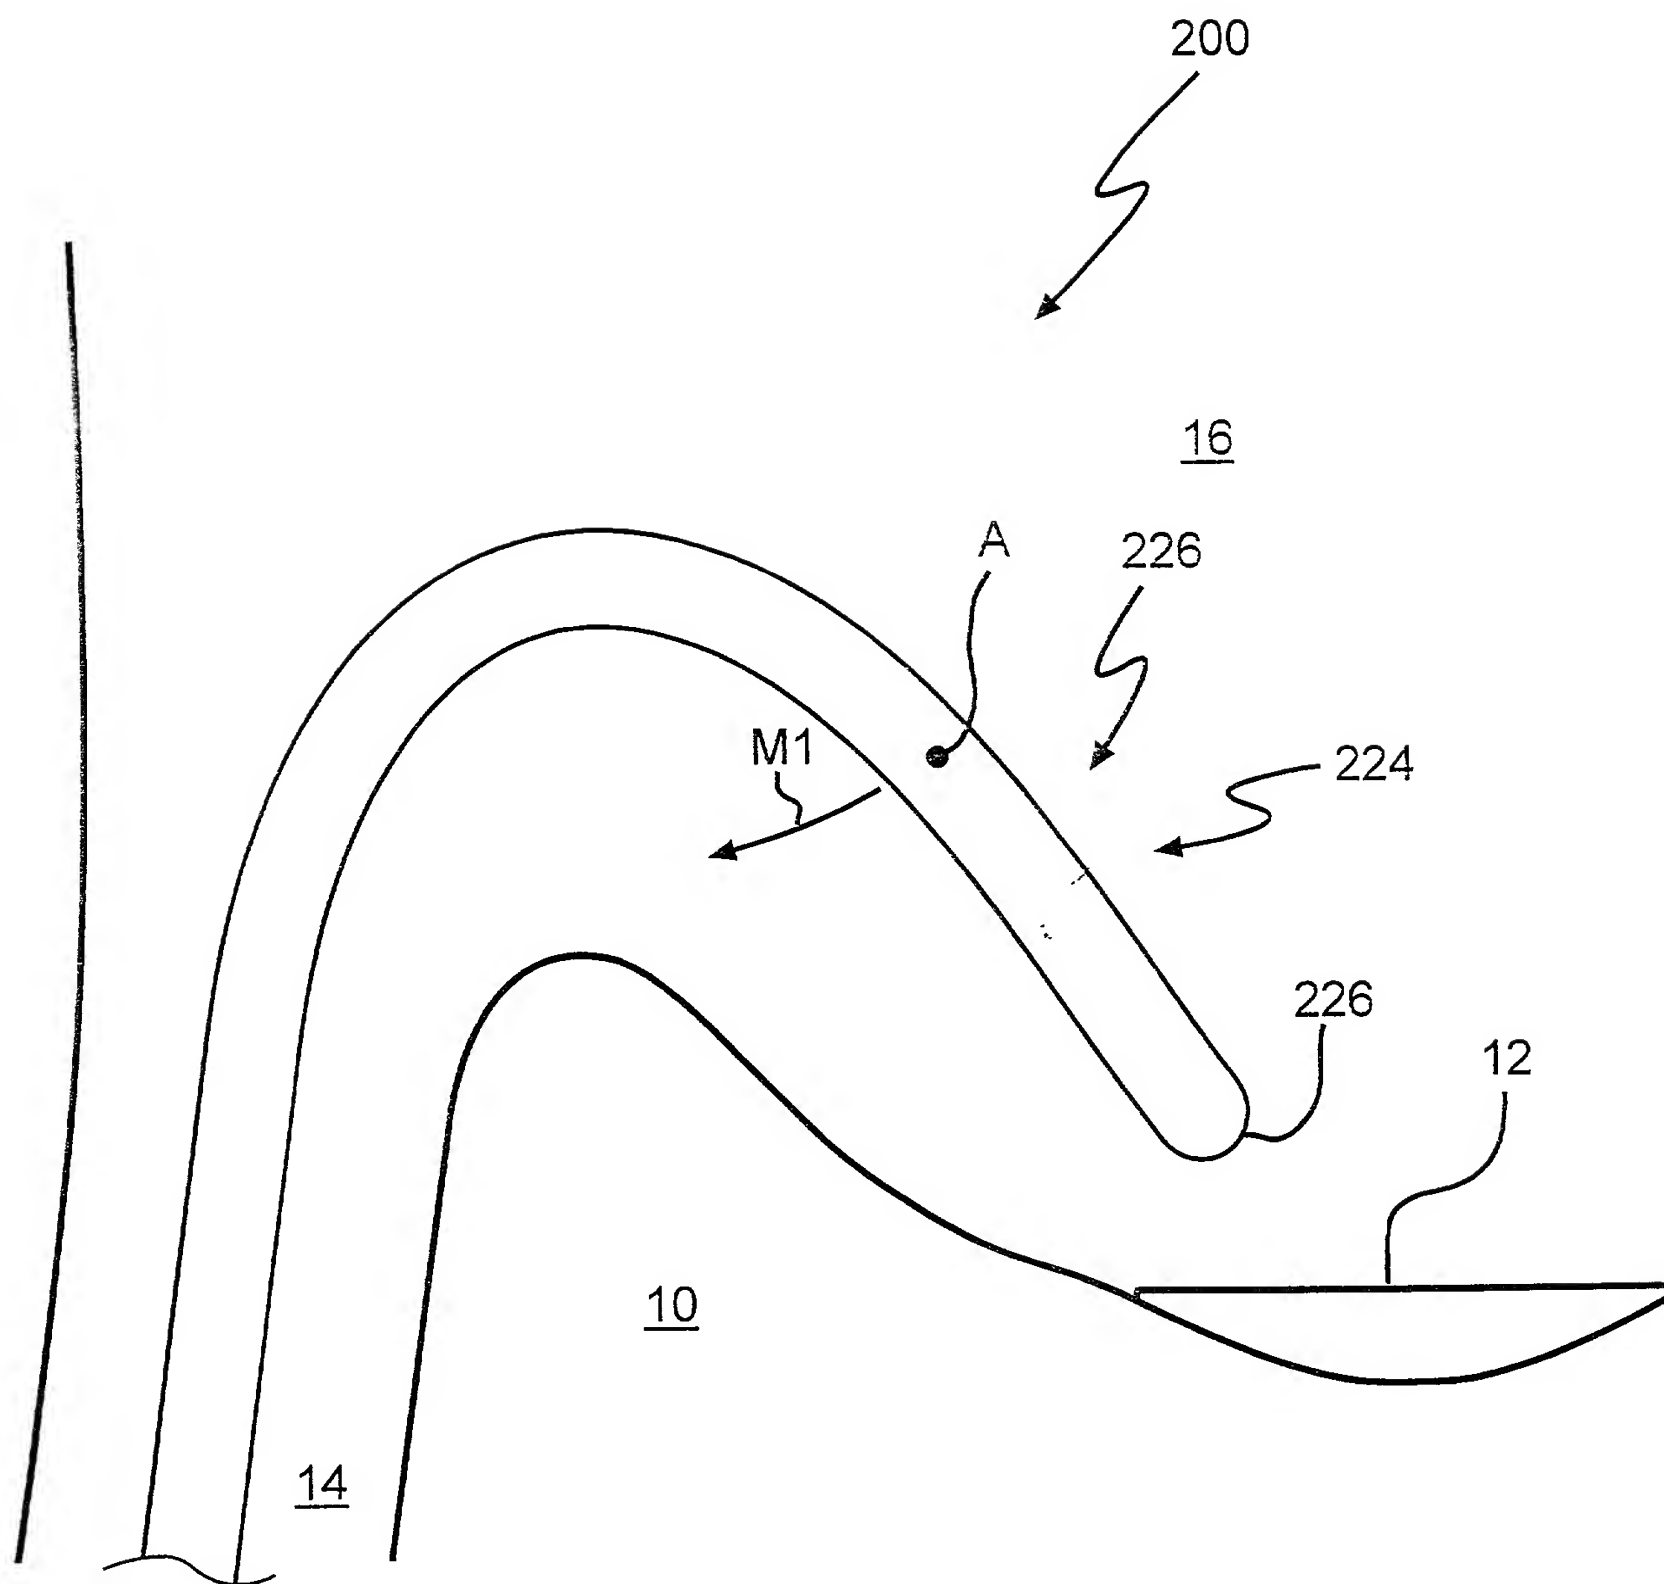

**FIG. 9B**

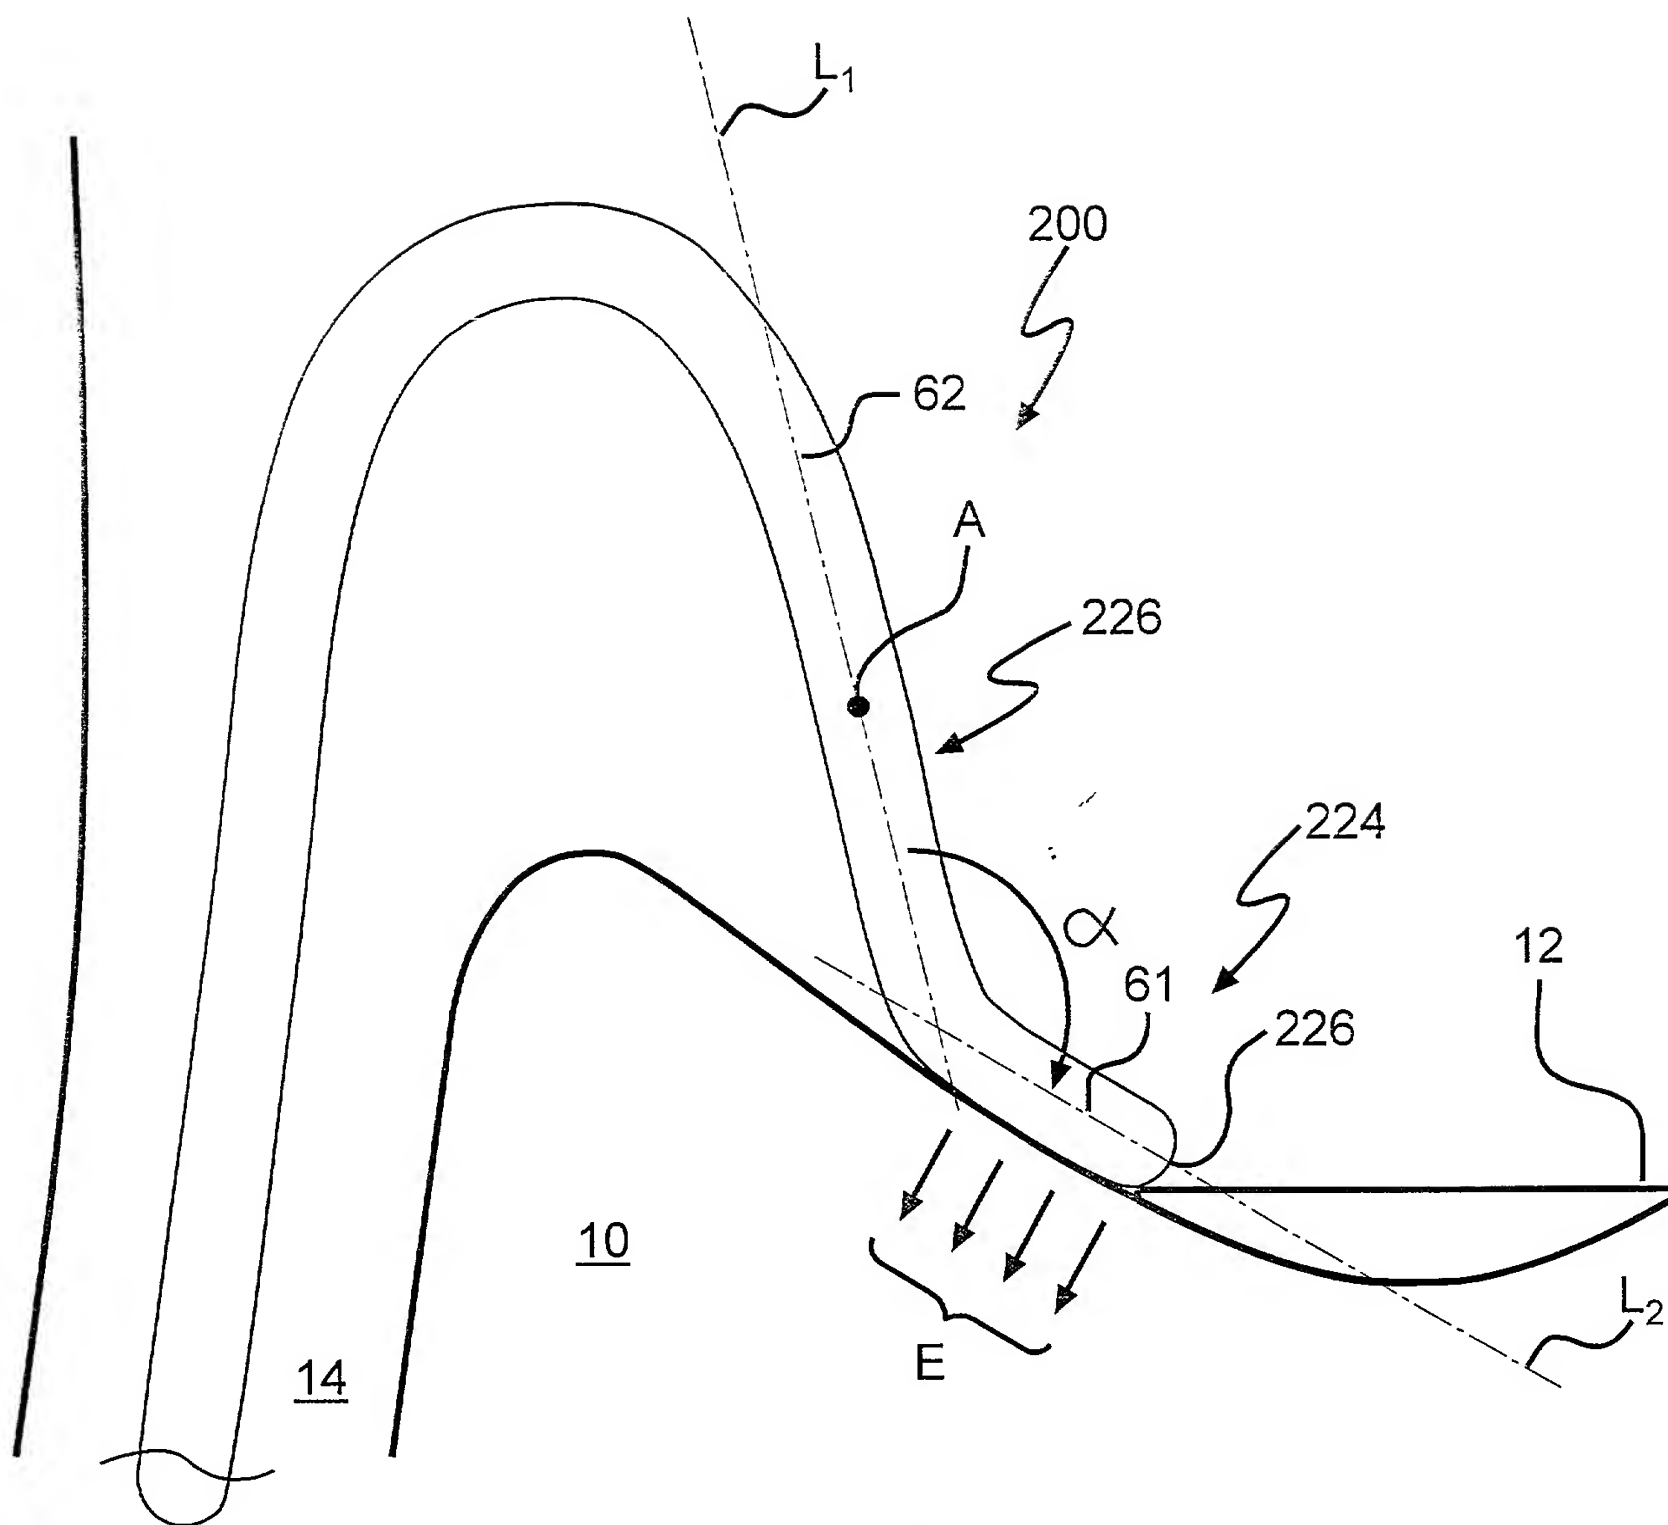

**FIG. 9C**



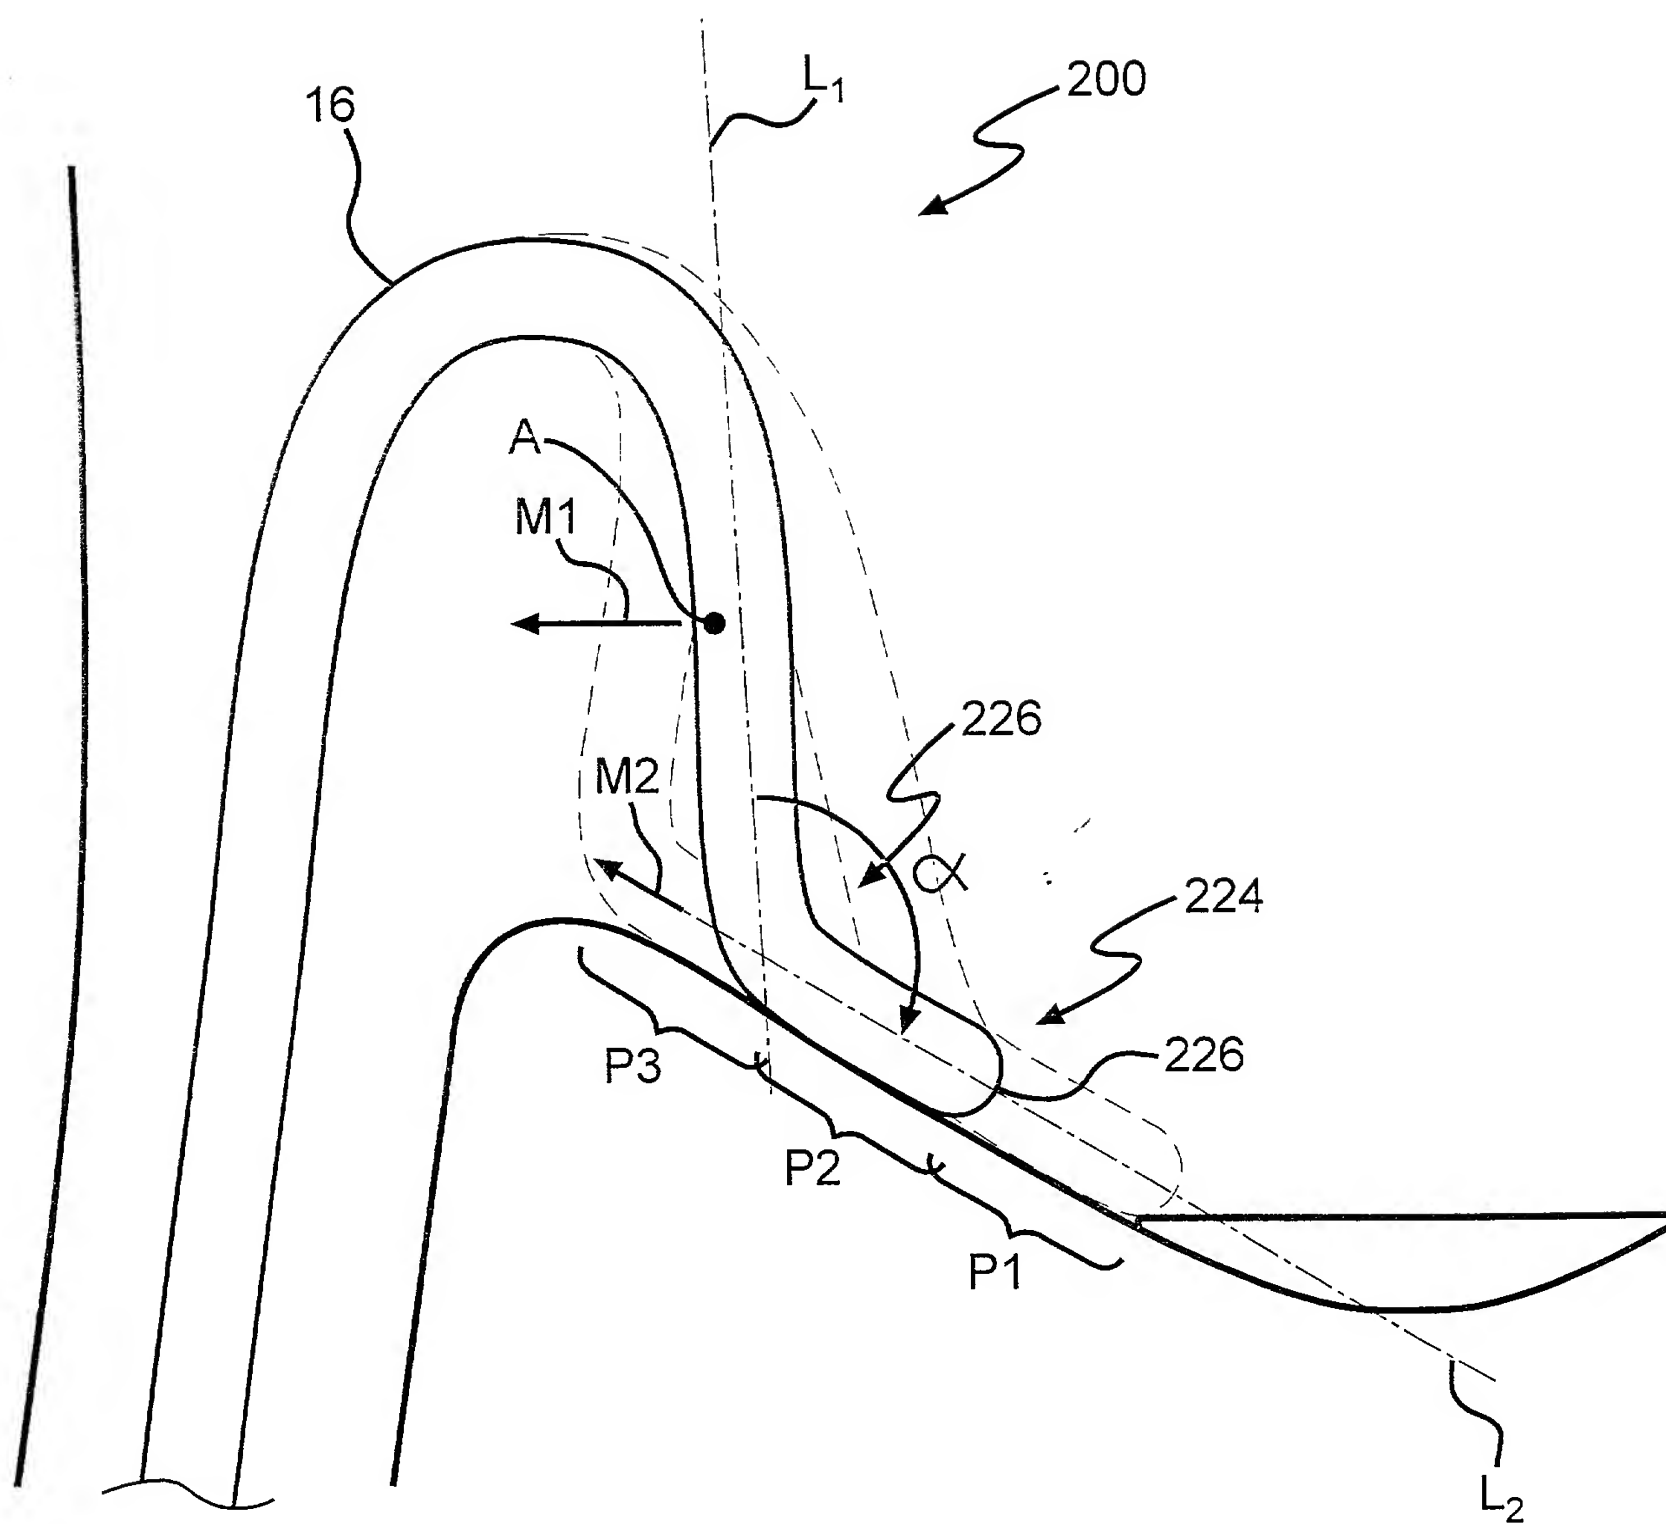


FIG. 9D

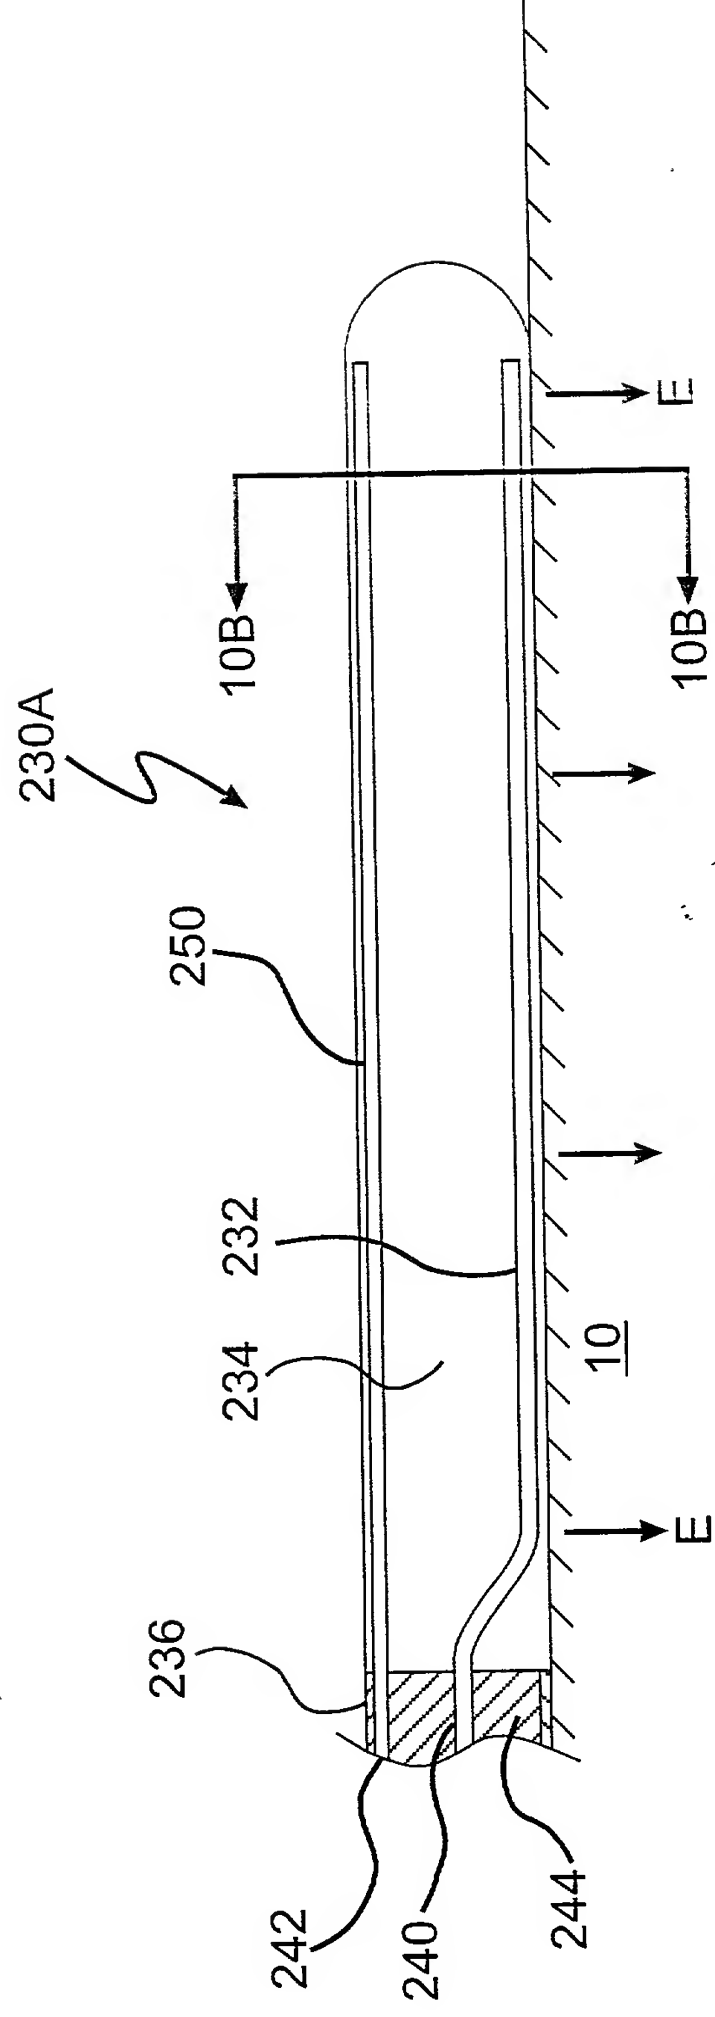

**FIG. 10A**

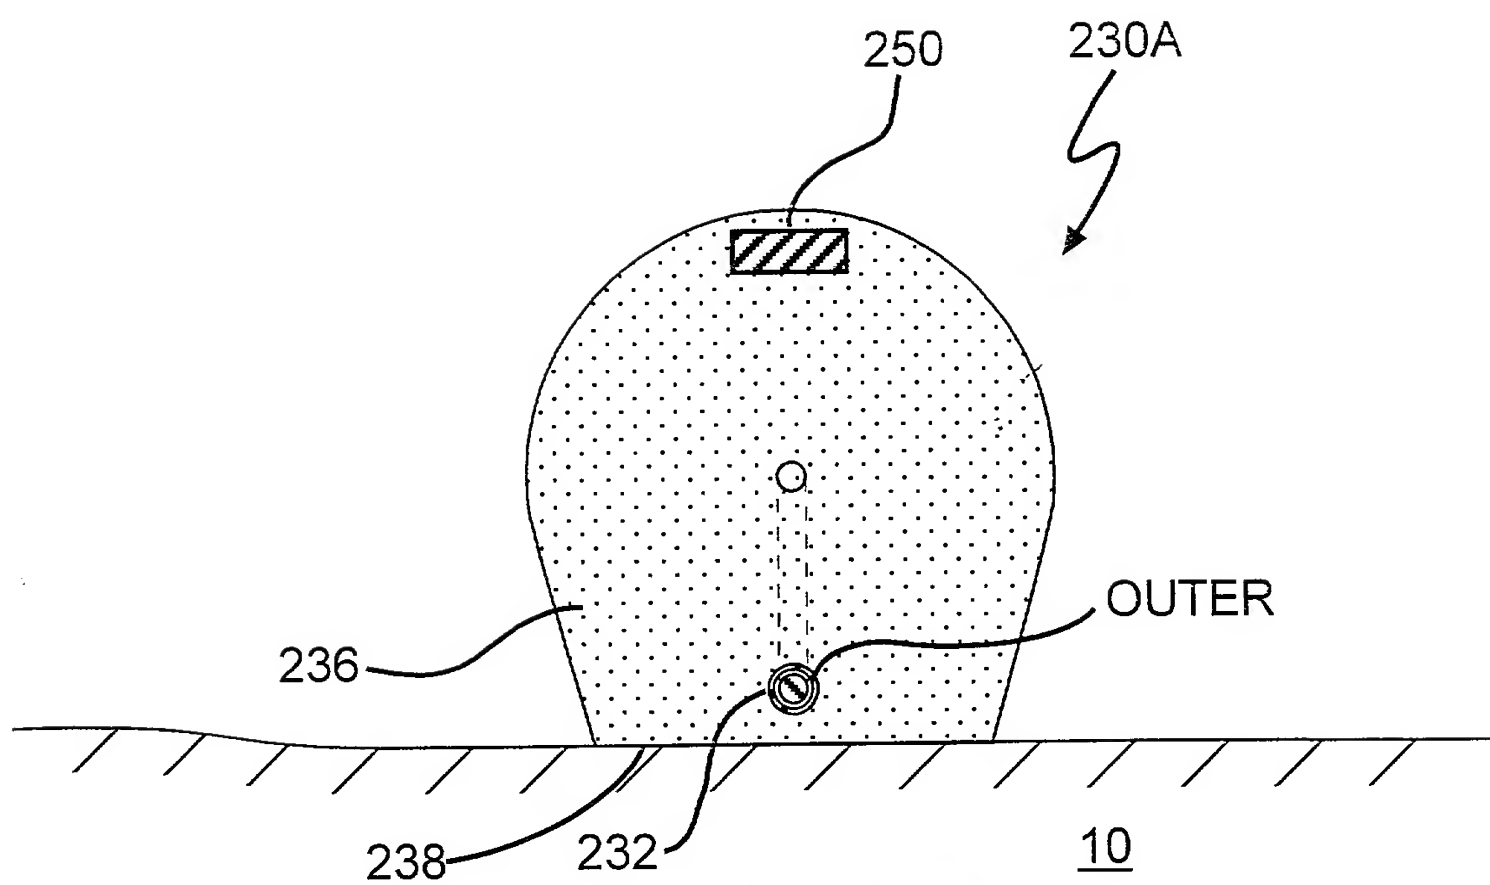

**FIG. 10B**


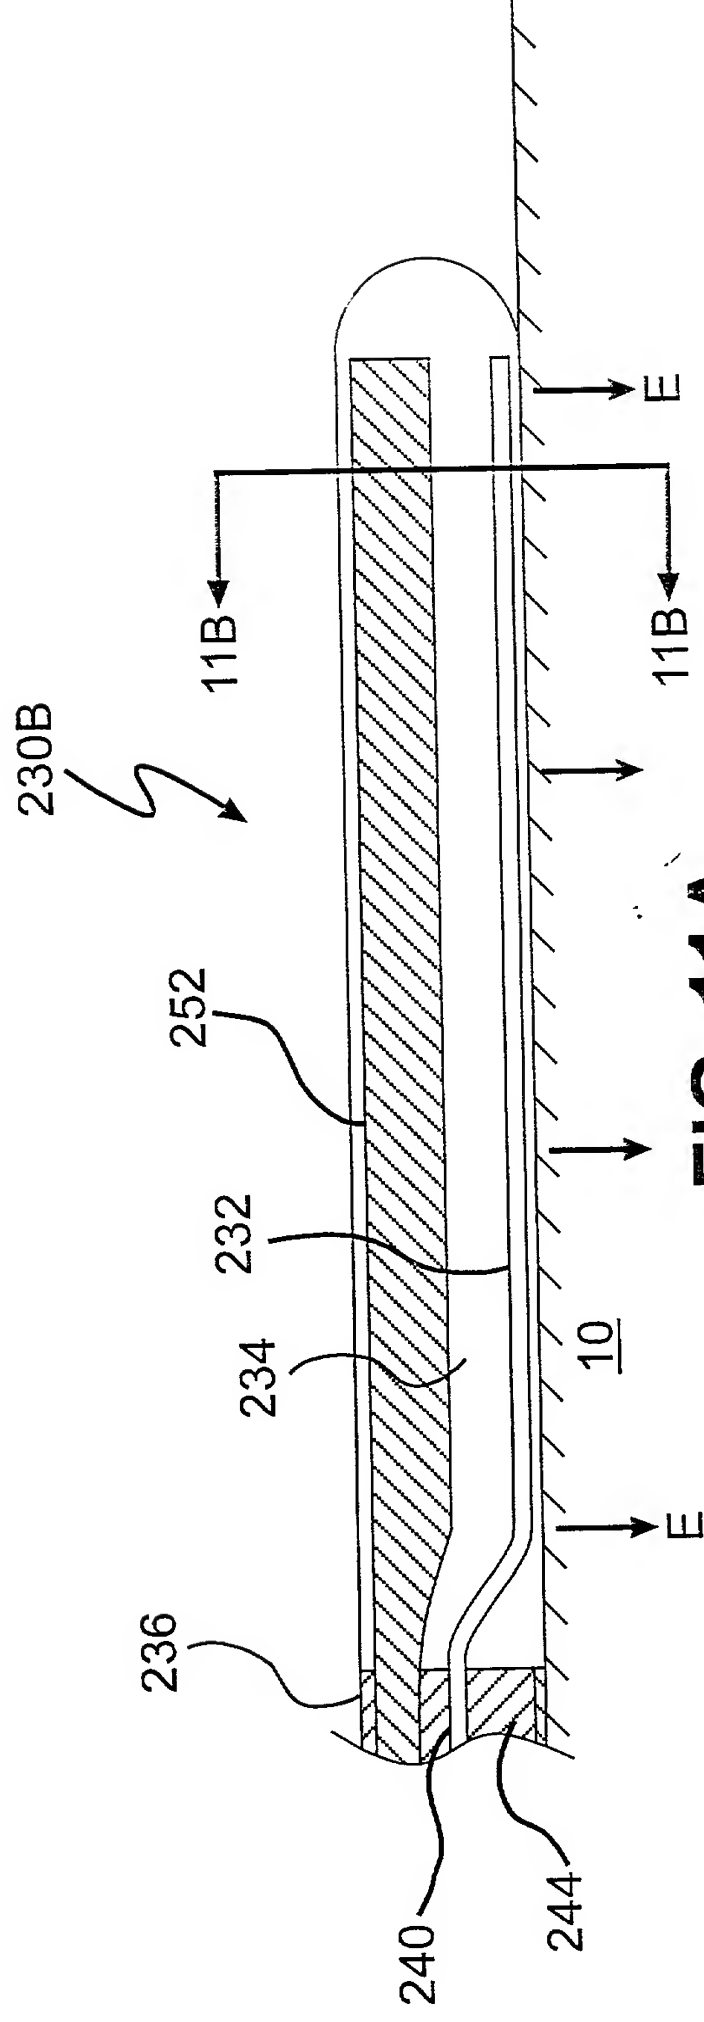


FIG. 11A

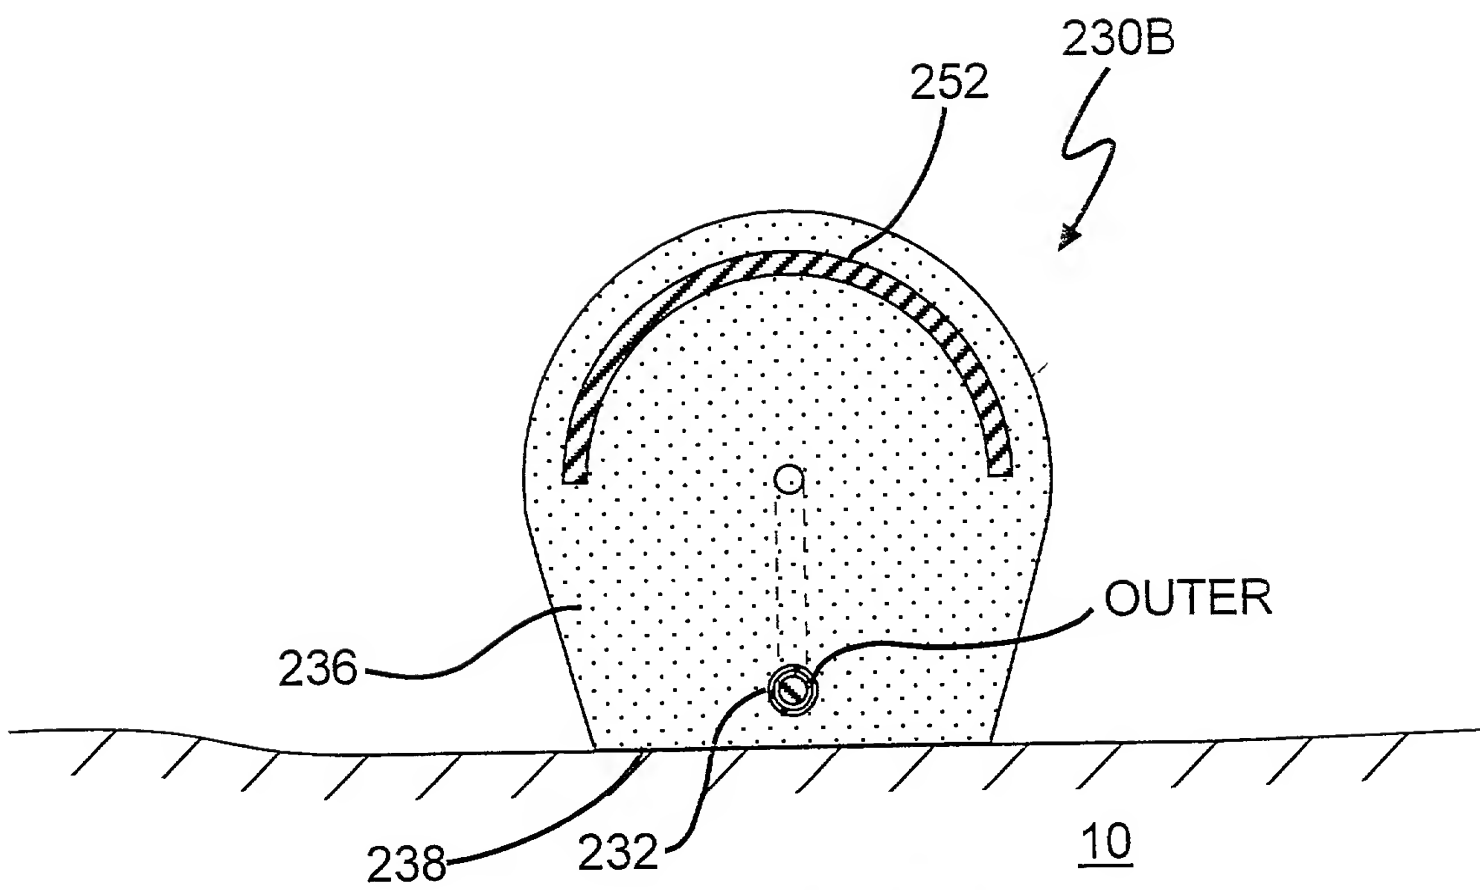

**FIG. 11B**